

MIS SEVEN Guide | 2014

mis[®]
User Manual

MIS scientists and engineers are continually seeking superior materials, technologies and procedures with the aim of developing quality products designed to make implant dentistry effective, safe and simple. The SEVEN implant system is one such breakthrough. With over ten years' proven clinical experience, the SEVEN has become the world's best-selling implant, providing a unique combination of surgical and restorative benefits.



© MIS Corporation. All Rights Reserved.






© MIS Corporation. All Rights Reserved.

MIS reserves the right to modify the products described in this manual as well as to revise this publication at any time and without informing any person of such revision or change. All Rights Reserved. No part of this publication may be reproduced, transcribed, stored in an electronic retrieval system, translated to any language or computer language, or transmitted in any form whatsoever without the written consent of the publisher. Questions, comments or requests will be addressed promptly by contacting MIS specialists directly through our e-mailing address: service@mis-implants.com. To learn more about MIS developments and products, visit our website at: www.mis-implants.com.

Note: This User Manual is for educational purposes only.



The MIS Quality System complies with International
Quality Standards: ISO 13485:2003 - Quality
Management System for Medical Devices.
ISO 9001: 2008 – Quality Management
System and CE Directive for Medical Devices
93/42/EEC. MIS products are cleared for
marketing in the USA and CE approved.

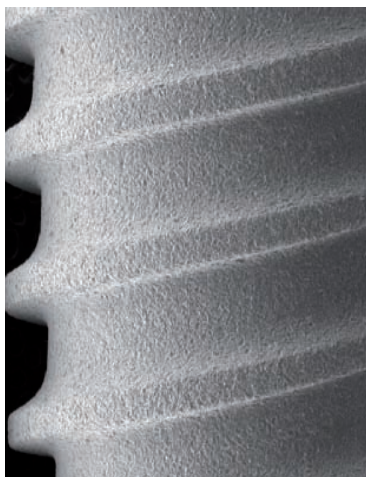



Overview.



- 8. Introduction
- 9. Raw Material
- 12. Manufacturing Process
- 13. Implant Surface
- 16. Histology
- 17. Hydrophilicity

Overview **Introduction**

MIS is a dynamic, state-of-the-art production company, developing and manufacturing a comprehensive range of dental implants designed to provide long-lasting successful solutions to partial and complete edentulous conditions. MIS implant systems combine several advantageous elements such as choice of raw materials, macro-structure, micro-structure and surface treatments, in order to achieve high primary stability and successful osseointegration.

MIS upholds high quality standards by conducting comprehensive quality assurance evaluations throughout the entire production process. MIS uses a clinically proven implant surface treatment technology that combines sand-blasting and acid-etching to increase surface area, creating both micro and nano-structures and eliminating surface contaminants. The implant surface is continuously monitored by a comprehensive series of tests, conducted both in-house and by internationally recognized research institutes. Tests include:

- Mechanical tests
- XPS analysis
- Roughness analysis
- Surface analysis
- SEM evaluations
- Cytotoxicity tests
- Sterility validations
- Torque removal values
- Histology

Overview **Raw Material**

- Biocompatible
- Safe
- Long-term proven clinical success
- Superior mechanical properties


All MIS implants are made from Ti-6Al-4V ELI (Grade 23), the higher purity version of Ti-6Al-4V. This specific type of alloy combines biocompatibility, excellent fatigue strength and low elastic modulus. These benefits make Ti-6Al-4V ELI mechanically superior to titanium grade 4 and the ultimate dental and medical titanium grade.

Ti-6Al-4V has been in use for over 25 years, and is the raw material most commonly used in the production of dental implants.

Similar to commercially pure titanium (Grades 1-4), the outer surface of all MIS implants are comprised of a thin layer of pure titanium oxide (TiO₂). In this way, bone cells cannot differentiate between the different titanium grades. The TiO₂ layer also prevents metallic ions leaking from the alloy, for safe long-term use.




Mechanical Properties
Raw Material

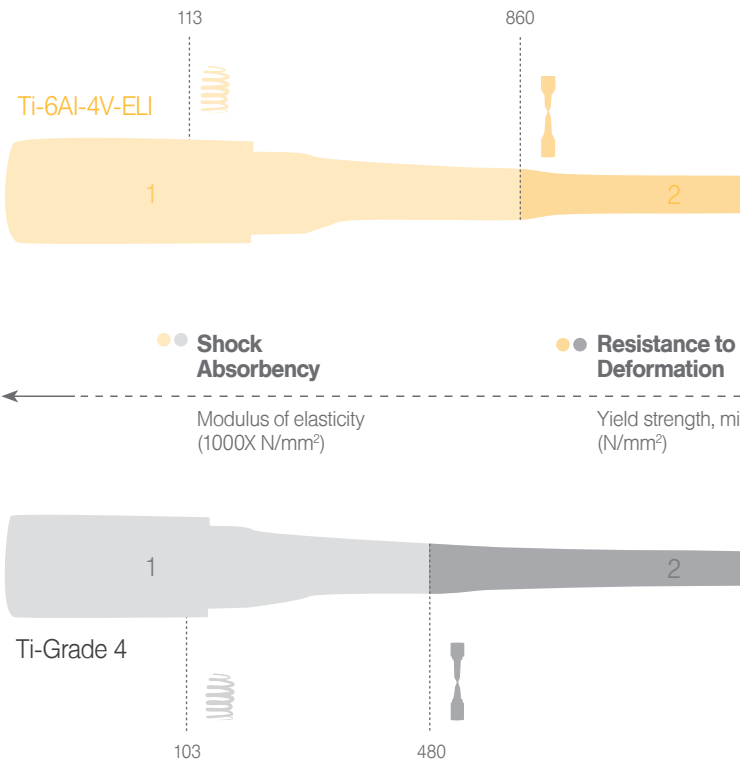

 Ti-6Al-4V-ELI = Ti-Grade 4

 Ti-6Al-4V-ELI > Ti-Grade 4

 Ti-6Al-4V-ELI > Ti-Grade 4

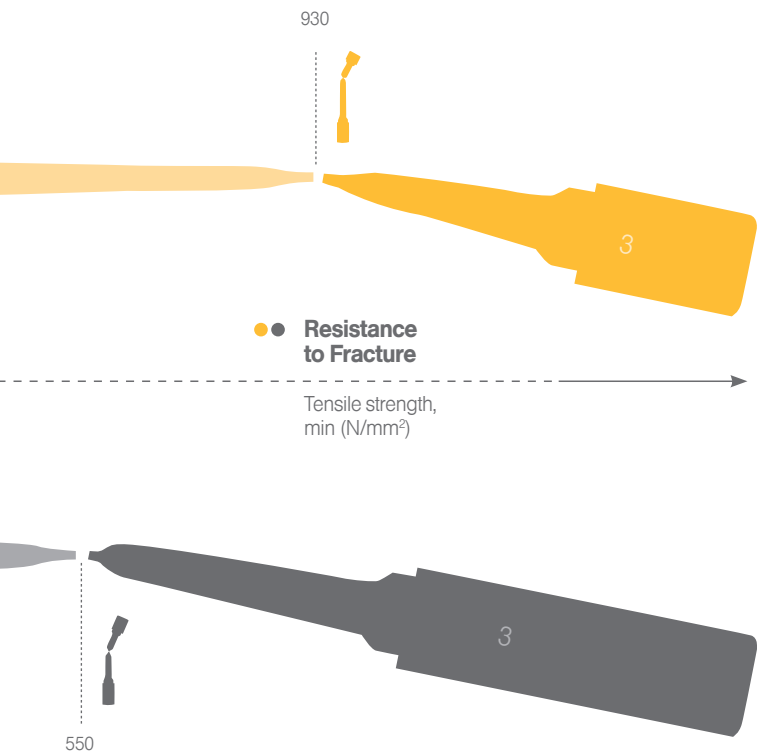

Overview
**Manufacturing
Process**



Structure (Raw Material)



MIS Surface Treatment



Sand-Blasting



Acid-Etching




Roughness (Macro and Nano Structures)


The combination of sand-blasting and acid-etching induces macro and nano-structures that significantly increase surface area of the implant body for optimal osseointegration. The roughened surface improves bone adhesion, as well as the proliferation and differentiation of osteoblasts.

Overview **Implant Surface**

Osseointegration is defined as the attachment of bone to dental implants, and is the critical factor related to the long-term success of dental implants. Osseointegration is determined by both the raw material of the implant, morphology and surface chemical composition.

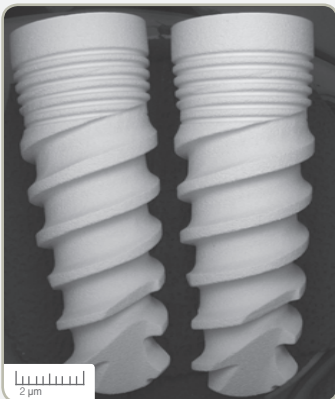

SEM image of two SEVEN implants

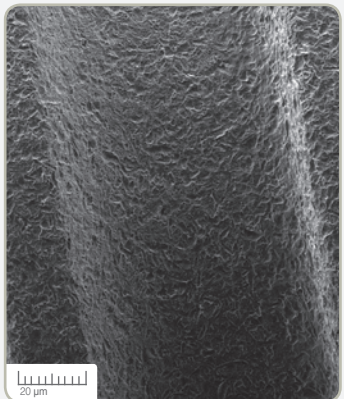

SEM image of the implant surface

Macro-structure

The geometric design of the body and thread profile of the implant act to increase primary stability and to distribute forces from the implant to the surrounding bone.

Micro and nano-structure


All MIS implants are sand-blasted and acid-etched. This surface treatment increases the implant surface area, creating both micro and nano-structures, while eliminating various surface contaminants.

MIS is one of only a handful of companies worldwide using electron microscopy on a daily basis for implant quality inspection.


Sand-blasted and acid-etched surfaces have been substantially proven to maximize the BIC (Bone-to-Implant Contact), achieving immediate and long-lasting osseointegration.

Surface composition


The outer surface of MIS implants, consist of a thin layer of pure titanium oxide (TiO_2). Acid-etching and packaging processes are performed in a controlled environment clean-room to ensure purity and quality. Implants are inspected by electron microscope (SEM) scan and X-ray photoelectron spectroscopy (XPS), to ensure implants are free of contaminants.

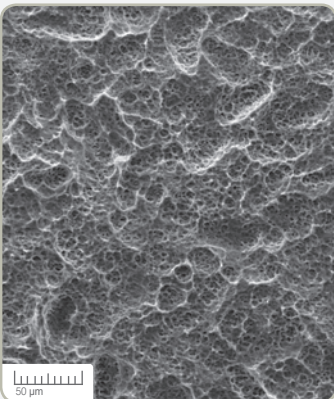

SEM image of the implant surface showing the micro-structure

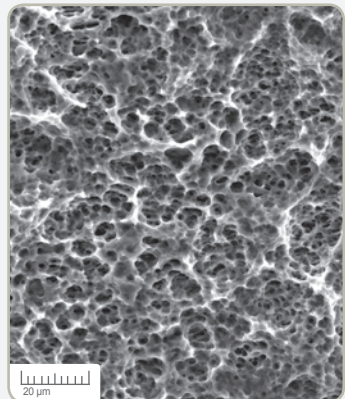


SEM image of the implant surface showing the nano-structure

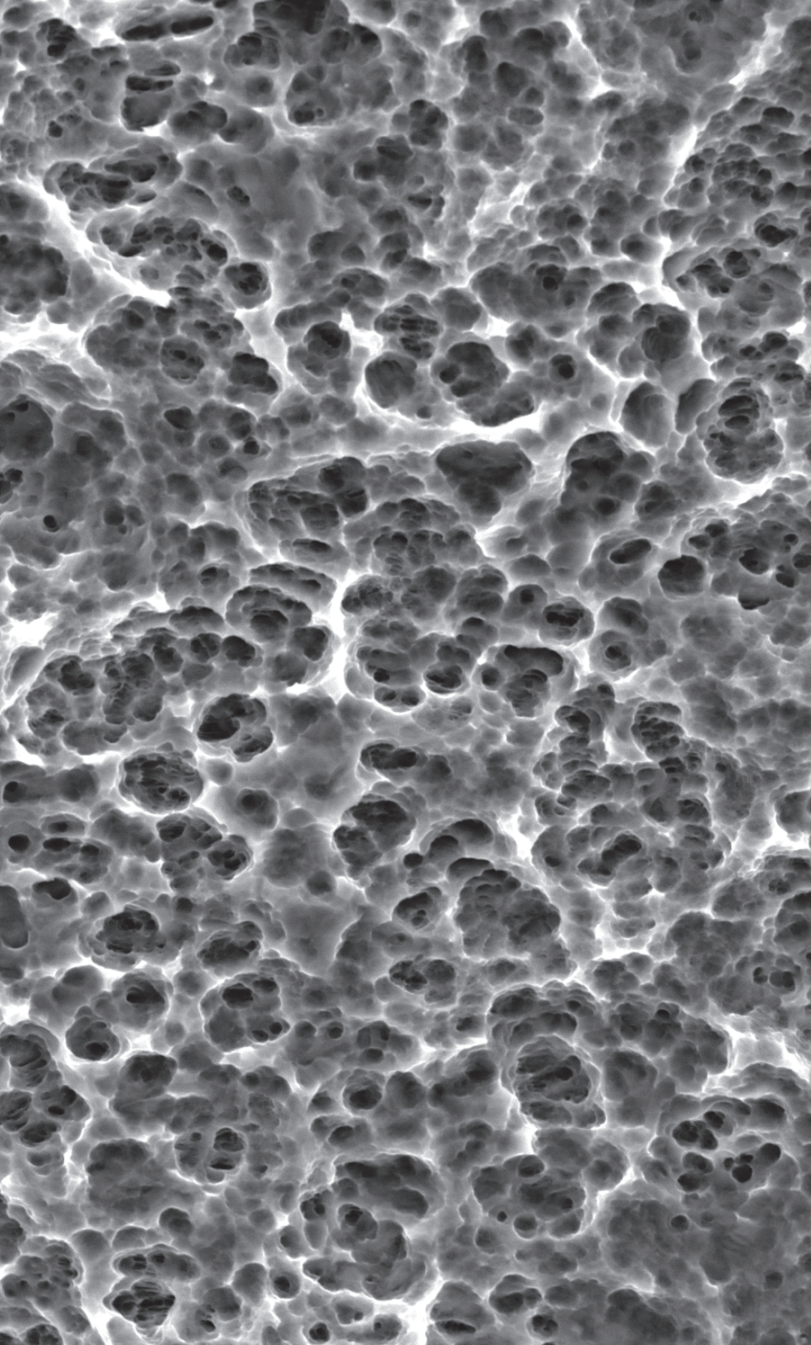

Overview **Histology**


Histologic section of a SEVEN implant, 5 weeks after placement. Courtesy of Paulo G. Coelho, DDS, PhD, NYU College of Dentistry.

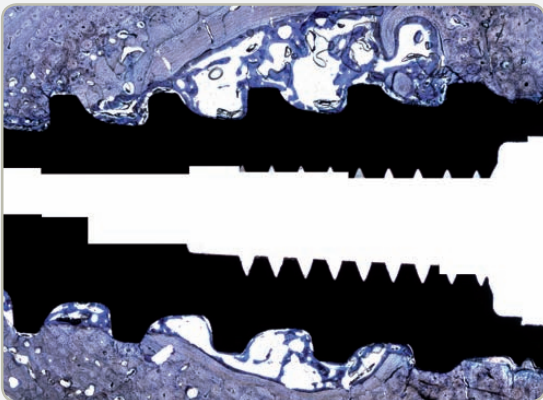


Courtesy of Paulo G. Coelho, DDS, PhD, NYU.

Overview **Hydrophilicity**

Current literature demonstrates a linkage between improved bone healing and early osseointegration with the hydrophilicity of surface. MIS implant surface treatment combines sand-blasting and acid-etching. This combination ensures surface purity and hydrophilic properties. The images demonstrate liquid "climbing" upwards on the implant surface.

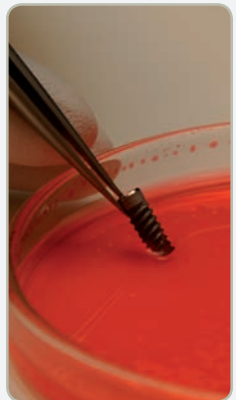

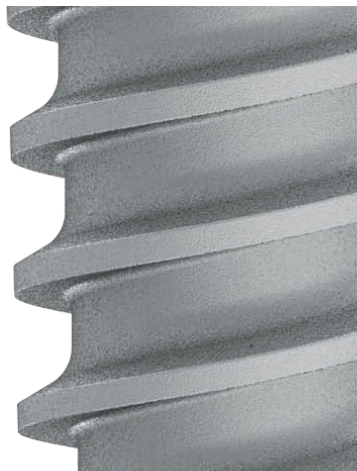



Implants.

- 20. Introduction: SEVEN Implant
- 21. Fixture - Technical Info
- 23. Features
- 24. Implant Range
- 25. Procedure

SEVEN


Introduction

The MIS self-tapping SEVEN implants are specially designed for use in a wide range of bone types and placement protocols. Their geometric design includes dual threads, spiral channels stemming from the apex, micro-rings on the implant neck and a changing thread thickness along the implant. All MIS SEVEN implants are supplied with a single use final drill, to ensure a sterile and consistently sharp blade for cutting bone walls to support the implant.




SEVEN NARROW

Fixture - Technical Info

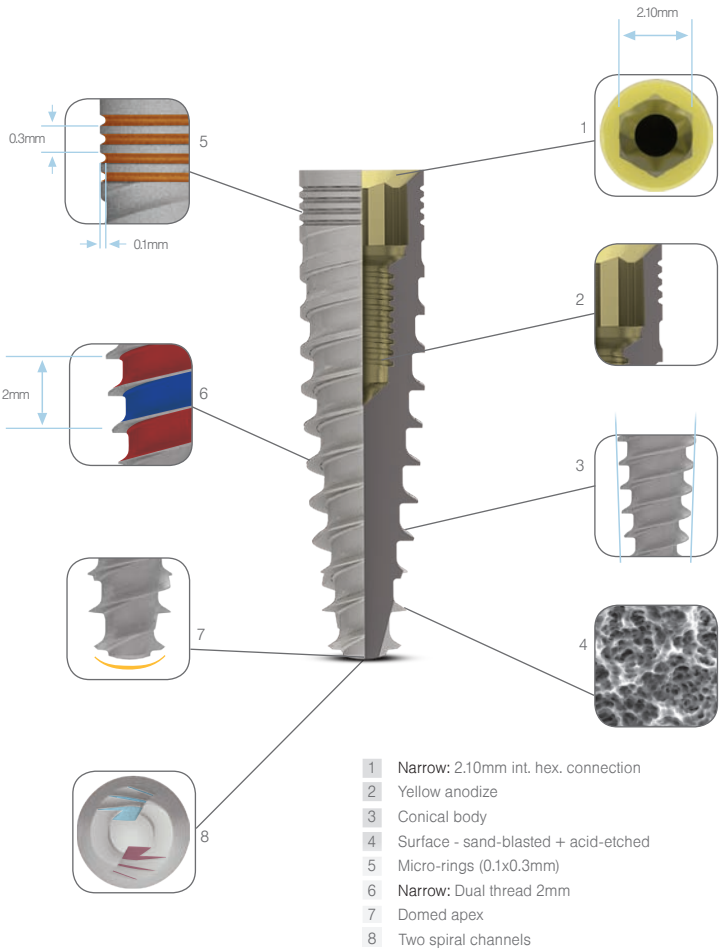

SEVEN STANDARD WIDE

Fixture - Technical Info

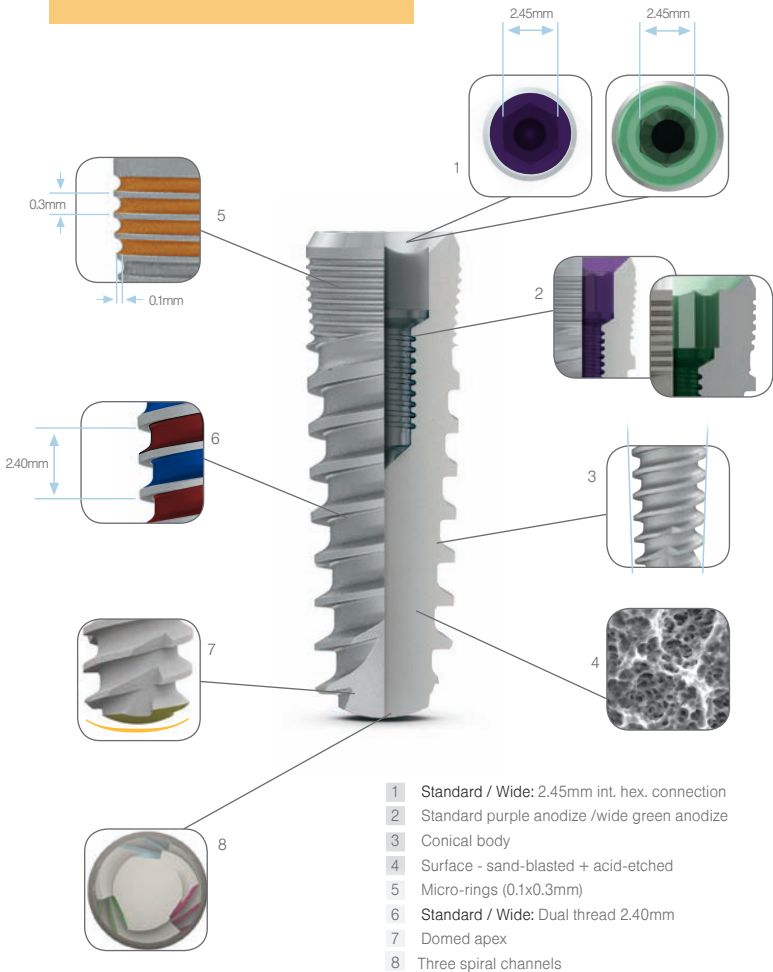

SEVEN

Features

Features

- The SEVEN implant is designed to suit a wide range of bone types and bone augmentation procedures.
- Specially designed final drill ensures shorter, safer drilling procedures.
- A double thread of 2.40mm increases implant insertion speed.
- Self-tapping capability.
- Three spiral channels for improved integration.
- The micro-rings (0.1x0.3mm) on the implant neck reduce stress in the crest zone.
- Differential thread thickness (0.15-0.4 mm) improves bone compression.
- SEVEN implants are available in 3.30, 3.75, 4.20, 5 and 6mm diameters and 6, 8, 10, 11.50, 13 and 16mm lengths.

Successful

The SEVEN implant has a high success rate as a result of its advanced geometric design and well-established surface morphology.

Versatile

SEVEN is designed for placement in a wide range of bone types and bone augmentation procedures.

Simple

Designed for a simpler and safer drilling procedure, every SEVEN implant is packed with a sterile, single-use final drill.

Efficient

The large thread design and self-tapping capability enables secure and fast implant insertion.

Primary Stability

Tapered thread thickness and depth, locks implant into the surrounding bone, to ensure smooth insertion and mild bone compression, resulting in high immediate stability.





Minimal Bone Resorption

The unique MIS surface treatment combined with micro-rings at the implant neck, ensure minimal bone resorption.

SEVEN

Implant Range

24.

Length	6mm	8mm	10mm	11.50mm	13mm	16mm
Ø3.30mm Screw type implant Narrow platform			MF7-10330 	MF7-11330 	MF7-13330 	MF7-16330 
Ø3.75mm Screw type implant Standard platform		MF7-08375 	MF7-10375 	MF7-11375 	MF7-13375 	MF7-16375 
Ø4.20mm Screw type implant Standard platform	MF7-06420 	MF7-08420 	MF7-10420 	MF7-11420 	MF7-13420 	MF7-16420 
Ø5mm Screw type implant Wide platform	MF7-06500 	MF7-08500 	MF7-10500 	MF7-11500 	MF7-13500 	MF7-16500 
Ø6mm Screw type implant Wide platform	MF7-06600 	MF7-08600 	MF7-10600 	MF7-11600 	MF7-13600 	

* Each SEVEN implant is supplied with a cover screw and a final drill.

SEVEN


Ø3.30mm / Ø3.75mm
Procedure

25.

* Recommended insertion torque: 35-60 Ncm.

Ø3.30mm Implant Procedure

Drilling Speed (RPM)	1200-1500	900-1200		200-400		15-25
Diameter	Ø1.90	Ø2.40	Ø2.40	Ø2.20 Ø3.20		Ø3.30

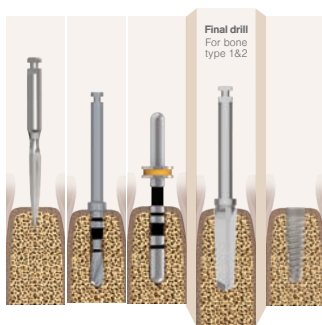


Do not use the final drill for bone type 3&4.

The drilling sequence is demonstrated by a 13mm implant.

Procedure recommended by MIS cannot replace the judgment and professional experience of the surgeon.

Ø3.75mm Implant Procedure

Drilling Speed (RPM)	1200-1500	900-1200		500-700		200-400	200-500		15-25
Diameter	Ø1.90	Ø2.40	Ø2.40	Ø2.80	Ø2.80	Ø2.80 Ø3.60	Ø3.75	Ø3.75	Ø3.75

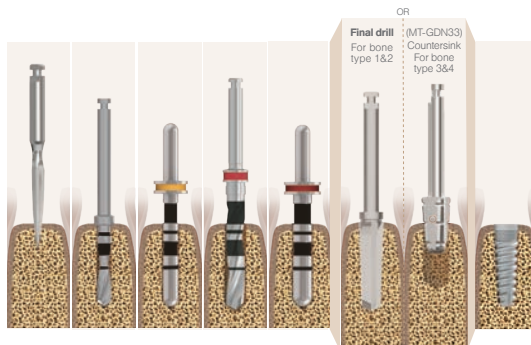


SEVEN

Ø4.20mm / Ø5mm
Procedure


26.

* Recommended insertion torque: 35-60 Ncm.

Ø4.20mm Implant Procedure

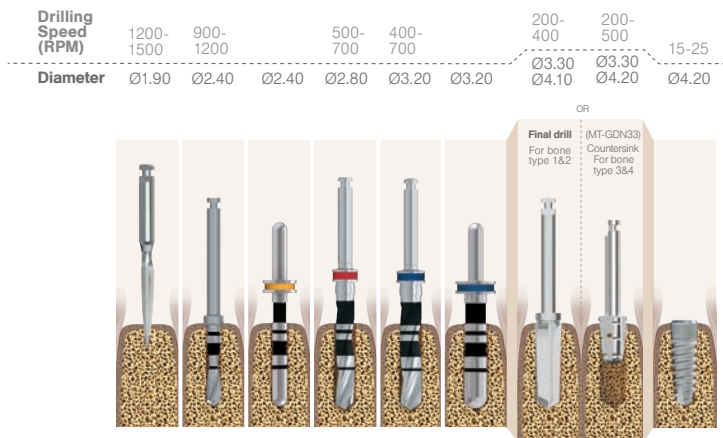

Ø5mm Implant Procedure

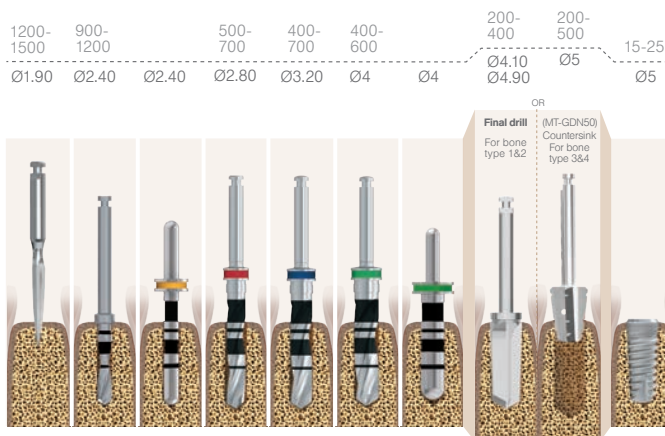




SEVEN

Ø6mm Procedure

* Recommended insertion torque: 35-60 Ncm.

Ø6mm Implant Procedure

Drilling Speed (RPM)	1200-1500	900-1200		500-700	400-700	400-600	300-500	300-500
Diameter	Ø1.90	Ø2.40	Ø2.40	Ø2.80	Ø3.20	Ø4	Ø4.50	Ø5

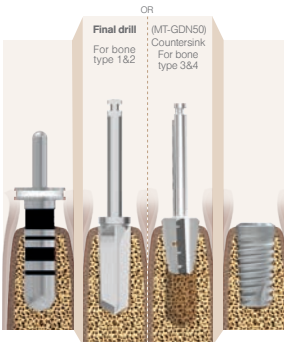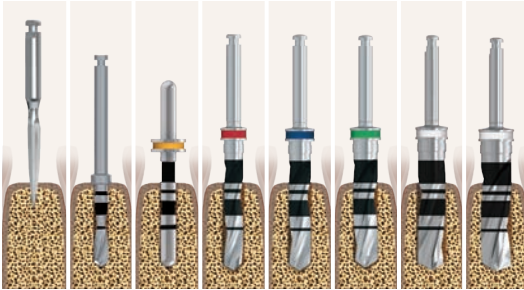

Do not use the final drill for bone type 3&4.

The drilling sequence is demonstrated by a 13mm implant.

Procedure recommended by MIS cannot replace the judgment and professional experience of the surgeon.



Surgical Procedures.

For MIS Implants

30. Indications and Contraindications

32. Step-by-Step Protocol

Surgical Procedures

Indications & Contraindications



Indications

Adequate bone is needed to support the implant with width and height being the primary dimensions of concern. The amount of available bone should be evaluated based on accepted imaging and radiological techniques used in implant dentistry.

In addition, a very careful evaluation has to be made as to the location of vital blood vessels, nerves, maxillary sinus, soft tissue spaces, and their relation to the site planned for implant placement.



Contraindications

All contraindications associated with elective surgery should be considered.

These include, but are not limited to:

- Metabolic bone diseases
- Blood and clotting disorders
- Medications affecting clotting or bone turnover
- Significant vascular or anatomic factors at the implant site
- Treatments, medications, or disorders that interfere with bone biology or wound healing.
- Hypersensitivity or known allergy to any components of the implants or their superstructures.



Other Contraindications

Poor patient motivation.

Psychiatric disorders that interfere with patient understanding and compliance with the necessary procedure.

Unrealistic patient expectations.

Unattainable prosthodontic reconstruction.

Inability of patient to manage oral hygiene.



Risks

Risks associated with the surgical procedure fall into four broad categories:

1. Immediate anesthetic and surgical risks.
2. Psychological and psychiatric risks.
3. Medical threats to long-term retention.
4. Long-term deleterious effects of implants on health.

The risks may include:

Inadvertent perforation of the nasal maxillary sinus, local and systemic infections, perforation into soft tissue spaces, rupture of primary blood vessels and nerve injury.

Temporary conditions that might result from implant placement may include pain and swelling, speech difficulties and haemorrhage.

Long term complications may include (but are not limited to) nerve injuries and persistent local or systemic infections. Special care and attention needs to be given to susceptible individuals with compromised immune systems due to medications, systemic conditions or those who underwent body part replacements.



Important Warning

Practitioner's lack of adequate training, knowledge and experience are considered major risk factors to the patient's health and to the implant's success. Therefore, no implant placement procedure should be performed without prior training by a certified institution.



Surgical Procedures

Step-by-Step Protocol

The surgical manual is designed to provide an overview of the pre-surgical and the surgical procedures applicable to the SEVEN implant range. Successful implant placement procedures are the result of a wide range of factors. This step-by-step protocol aims to ensure that significant factors are not overlooked.



Step 1.

Patient Selection and Medical History
(General medical history)

Patients must be carefully assessed for their ability to safely undergo surgical procedures. Medical history should be evaluated to ensure that patients are not put at risk. Certain medical conditions are considered either absolute or relative contra-indications for surgery. These may involve (but are not limited to) the following conditions: patients who are either taking or took medications for the treatment of osteoporosis; immunodeficiency or immunosuppressive

treatments; malignancies; head and neck radiation; poorly controlled diabetes or other hormonal disorders; bleeding disorders or anticoagulant therapy; recent myocardial infarction, severe cardiac insufficiency and valve pathology; general bone diseases; hypersensitivity or known allergy to specific relevant materials; psychiatric or personality disorders that limit or interfere with patients' understanding and compliance. Please be aware of the fact that updates based on current medical literature may include or exclude certain conditions.



Step 2.

Dental Conditions and Oral Hygiene

A complete and thorough intraoral examination must be performed and recorded. This must include an evaluation of the dentition, oral hygiene, smoking, habits, attitude to oral health, and any other relevant information. Implant procedures should not be performed on patients with active osteolytic conditions, active periodontal disease or infectious areas at the implant site. Extreme bruxing and clenching should be taken into consideration.



Step 3.

Radiographs and Imaging

Diagnosis and treatment planning for implant placement require the use of different types of radiographs and imaging technologies. Panoramic radiographs are considered standard pre-surgery radiographs, however additional imaging modalities such as CT (Computerized Tomography), Tomography and periapical radiographs may be required.

It should be emphasized that certain countries require specific radiographs to be taken in advance.

during and after surgery. It is the obligation of the surgeon to ensure that all required documentation is available and recorded before and after surgery. Vertical and horizontal dimensions of implant sites should be measured and charted. The anatomical relationships of neighboring teeth and proximity to anatomical structures such as the mandibular canal, maxillary sinus and base of the nose must be evaluated. Bone inclination and shape should also be taken into account. Surgical guides with radioopaque markers are recommended. These, coupled with computerized tomographic radiographs can later be altered to be use as computer-based surgical guides.



Step 4.

Treatment Plan (Patient cooperation)

Based on patient's needs, alternative treatment plans should be considered and discussed. The chosen treatment plan should result in a sequence of actions related to initial preparations, surgical phase and a restorative phase.

Surgical Procedures

Step-by-Step Protocol



Step 5A.

Implant Selection

SEVEN implants feature a range of diameters and lengths. It is recommended that Wide platform implants are used in the premolar and molar areas, while Standard platform implants are used in the anterior areas. Specific analysis of available bone and distance from vital structures at each proposed site may lead to the choice of specific implant length and diameter; however, current augmentation procedures may allow the use of longer or wider implants.



Step 5B.

Surgical Phase

Surgery should be performed under strict infection control conditions. Preoperative medications and/or antibiotics may be required based on the patient's condition and the extent of surgery, and should be decided upon by the operating surgeon. Other monitoring measures, including blood-pressure and pulse measurements should also be considered. Emergency resuscitation apparatus should be available. Each MIS implant comes with labels including all relevant data related to the implant. It is critical that the label is kept as part of the patient's record for future reference.

Warnings: SEVEN implants are supplied in a sealed and sterilized package. Implants should never be reused, and implants whose sterility is compromised should not be used. Implants should not be used later than the specific expiration date printed on the package. Implant placement should be performed in accordance with acceptable placement and loading protocols. Recommended MIS procedures are described on pages 20-43. However, it should be emphasized that procedures recommended by MIS

cannot replace the judgment and professional experience of the surgeon. The sale of MIS implants is restricted by law to licensed dentists only. Implant placement procedures should only be performed by trained and licensed dentists. Initial planning is of the utmost importance. As this is a prosthetic driven procedure, it is advisable that the restorative dentists be involved at the planning and the surgical phases as active participants when making decisions affecting the choice of implant type and the three dimensional positioning of the implant.

12 24

Step 6. Osseointegration Phase

Current literature supports multiple loading options. Dentist should decide when to load implants based on specific parameters, related to their individual case.



Step 7. Restorative Phase

SEVEN implants can support different types of final restorations. Following the solution specified in the treatment plan, the final restoration is fabricated based on accepted restorative protocols. Special attention should be given to ensure correct occlusal adjustment, in order to prevent overloads on the implant supported restorations. MIS superstructures and components must be used with all MIS implants.



Step 8. Follow-up

Annual follow-up evaluations including radiographs are required. Special emphasis should be put on oral hygiene and habits, occlusion adjustments and the stability of the prosthesis.





Surgical Kit.

- 38. Surgical Kit Description
- 40. Advanced Surgical Instrument Kit
- 42. Kit Contents

The Surgical Kit

Surgical Kit Description

The SEVEN surgical kit comprises a complete range of drills and tools required for SEVEN implant placement procedures. It features a convenient ergonomic layout that follows the surgical drilling sequence, and includes a set of length-based pilot drills for a smoother more accurate procedure. Kit components are color-coded for immediate identification of diameters for both implants and restorative platforms.



▲ **MK-EI48**, advanced surgical kit for SEVEN implant system with external irrigation drills



Please Note:

The surgical kit is made of medically approved materials.

The surgical kit can be fully sterilized using a pre-vacuum autoclave at temperatures that do not exceed 132°C (270°F) for 4 minutes.

The surgical kit is compact and easy to store.

Tray can be removed from the box for easy cleaning and sterilization.

Steam flow is optimized through built-in vents.



Warning

Avoid damage!

Temperatures higher than 150°C may cause damage. Radel, steel and silicone components may support repeated exposure to temperatures up to 180°C, however tray-life may be reduced.

The use of cleaning or disinfecting agents containing high rates of chlorine or oxalic acid may cause damage to the trays and to the instruments. Please handle with care to avoid breakage. Never use broken trays or instruments.

Do not open the box while still hot after sterilization.



Cleaning Procedure

Stainless steel instruments should be cleaned and sterilized with materials that are specifically

indicated for these materials. To avoid damage, please refrain from using:

- Cleaning and disinfection agents containing high rates of chlorine
- Cleaning or disinfection agents containing oxalic acid.

In order to prevent damage to instruments that are color-coded, please refrain from using:


- Detergents and cleaning agents containing high rates of the aforementioned chemicals
- Extremely high temperature during cleaning and sterilization.


Please Note:

- Please conduct a visual inspection of the instruments prior to each use. Do not use faulty and dull instruments. Clean and disinfect each instrument separately
- Do not allow traces/residue (blood, secretion, tissue residue) to dry on the instruments. Always soak in disinfecting fluid immediately after use
- Use only stainless steel dedicated detergents and strictly follow usage instructions
- Rinse instruments thoroughly with water to remove any remaining disinfectants or cleaning agents
- Do not store instruments that are damp or wet
- Use only nylon bristle brushes to clean instruments. Clean the cavities and hollow spaces thoroughly
- The use of an ultrasonic bath is highly recommended
- Do not clean/ disinfect instruments made of different materials together
- To prevent damage, do not allow sharp instruments to touch other instruments during cleaning
- After mechanical or manual cleaning, all surgical instruments must be sterilized in an autoclave, at 134°C (273°F), pressure of ≈315 Kpa for 6 minutes or in a pre-vacuum autoclave at 132°C (270°F) for 4 minutes. Do not exceed 134°C. Never use dry sterilizers
- Inspect for corrosion after sterilization.

The Surgical Kit
**Advanced
Surgical
Instrument Kit**

MK-EI48 | With external irrigation drills

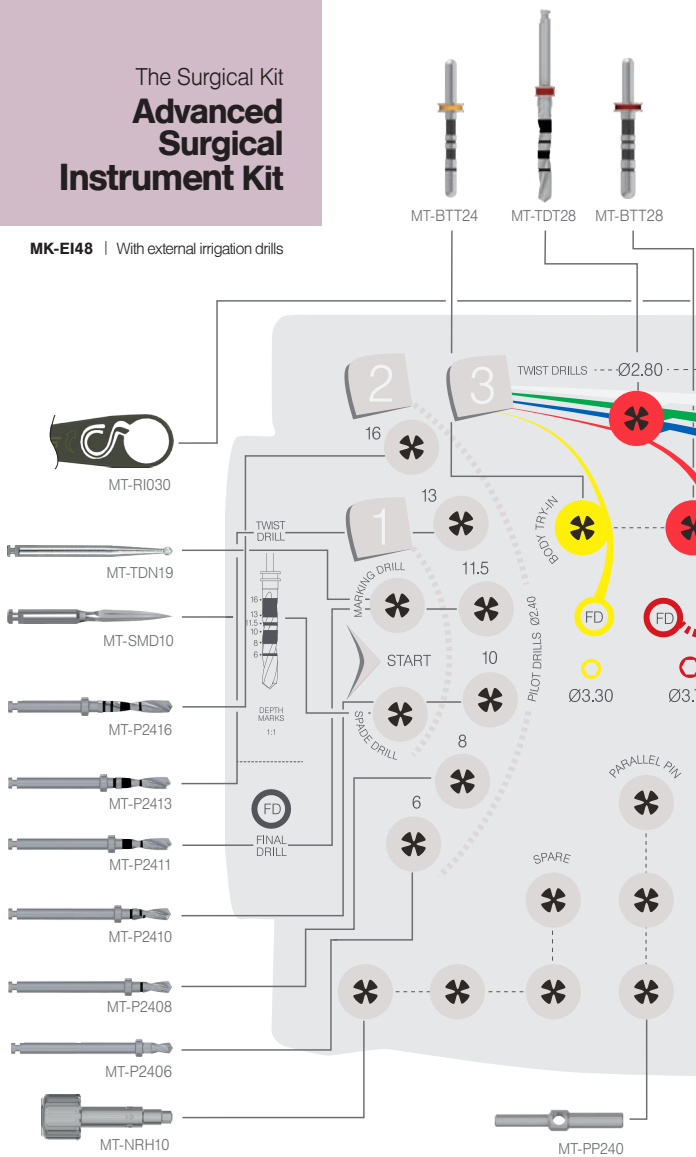

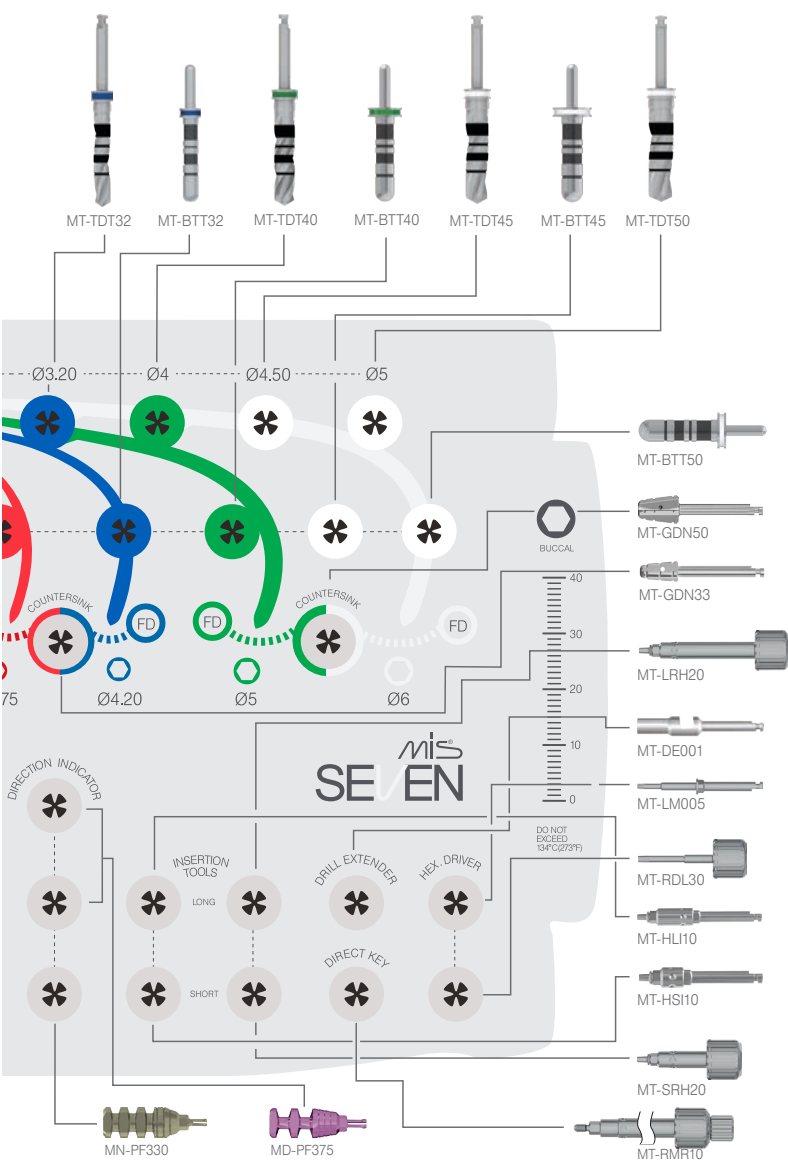

The Surgical Kit Kit Contents

The SEVEN Surgical Kit contains tools specifically designed for a step-by-step placement process. Correct preparation of the implant site ensures efficient and accurate placement and high primary stability.


























The Surgical Kit
Kit Contents



		Dimensions	Material
	MT-P2406 Pilot drill with built in stopper Ø2.40 height 6mm	Ø2.40mm Length 31mm	Stainless steel
	MT-P2408 Pilot drill with built in stopper Ø2.40 height 8mm	Ø2.40mm Length 31mm	Stainless steel
	MT-P2410 Pilot drill with built in stopper Ø2.40 height 10mm	Ø2.40mm Length 31mm	Stainless steel
	MT-P2411 Pilot drill with built in stopper Ø2.40 height 11.5mm	Ø2.40mm Length 31mm	Stainless steel
	MT-P2413 Pilot drill with built in stopper Ø2.40 height 13mm	Ø2.40mm Length 31mm	Stainless steel
	MT-P2416 Pilot drill with built in stopper Ø2.40 height 16mm	Ø2.40mm Length 31mm	Stainless steel
	MT-BTT24 Body try-in Ø2.40mm for tapered impl. procedure	Ø2.40mm Length 28.5mm	Stainless steel
	MT-BTT28 Body try-in Ø2.80mm for tapered impl. procedure	Ø2.80mm Length 28.5mm	Stainless steel
	MT-BTT32 Body try-in Ø3.20mm for tapered impl. procedure	Ø3.20mm Length 28.5mm	Stainless steel
	MT-BTT40 Body try-in Ø4mm for tapered impl. procedure	Ø4mm Length 28.5mm	Stainless steel
	MT-BTT45 Body try-in Ø4.50mm for tapered impl. procedure	Ø4.50mm Length 28.5mm	Stainless steel
	MT-BTT50 Body try-in Ø5mm for tapered impl. procedure	Ø5mm Length 25.5mm	Stainless steel
	MT-TDT28 Twist drill 2.80mm external irrigation	Ø2.80mm Length 37.5mm	Stainless steel

The Surgical Kit Kit Contents

		Dimensions	Material
	MT-TDT32 Twist drill 3.20mm external irrigation	Ø3.20mm Length 375mm	Stainless steel
	MT-TDT40 Twist drill 4mm external irrigation	Ø4mm Length 382mm	Stainless steel
	MT-TDT45 Twist drill 4.50mm external irrigation	Ø4.50mm Length 382mm	Stainless steel
	MT-TDT50 Twist drill 5mm external irrigation	Ø5mm Length 382mm	Stainless steel
	MT-SMD10 Spade marking drill	Length 275mm	Stainless steel
	MT-TDN19 Marking drill Ø1.90mm external irrigation	Ø1.90mm Length 34mm	Stainless steel
	MT-LRH20 Long insertion tool for int. hex. connection	Length 32.3mm	Stainless steel
	MT-NRH10 Long ratchet adapter for int. hex. connection, NP	Length 24.5mm	Stainless steel
	MT-LM005 Long motor adapter for 0.05" hex.	Length 30mm	Stainless steel

			Dimensions	Material
	MT-RDL30	Long hex. drive 0.05 inch	Length 23.5mm	Stainless steel
	MT-DE001	Drill extender	Length 24mm	Stainless steel
	MT-PP240	Parallel pin Ø2.40mm for tapered impl. procedure	Ø2.40/ Ø3mm / Length 24mm	Stainless steel
	MN-PF330	Direct press fit for closed tray NP	Length 16.7mm	Titanium
	MD-PF375	Direct press fit for closed tray	Length 16.3mm	Titanium
	MT-HSI10	Short insertion tool, int. hex. connection	Length 24.4mm	Stainless steel
	MT-HLI10	Long insertion tool, int. hex. connection	Length 28.2mm	Stainless steel
	MT-SRH20	Short insertion tool for int. hex. connection	Length 22.30mm	Stainless steel
	MT-RMR10	Long direct hand and ratchet key	Length 38.50mm	Stainless steel
	MT-GDN33	Countersink for Standard platform implant system	Ø3.75mm/ Ø4.20mm Length 26mm	Stainless steel
	MT-GDN50	Countersink for Wide platform implant system	Ø3.75mm/ Ø4.20mm Length 26mm	Stainless steel
	MT-RI030	Ratchet wrench	Length 84mm	





Drills.

- 50. Use of MIS Drills
- 52. Color Code
- 54. Drill Indications
- 56. Overview
- 58. Final Drill
- 60. Countersink Drills
- 61. Ceramic Drills
- 62. Drill Maintenance

Drills


Using MIS Drills

Implant placement procedures require the use of several drills with different diameters and characteristics. MIS offers drills with internal and external irrigation, as well as conical and ceramic drills. Most MIS drills are marked for depth control and are color coded for immediate identification of drill diameter.

Features

MIS drills are designed to be used with all MIS implants. Drills are available with or without internal irrigation. Short drills are also available for each diameter. All drills are color-coded. The drills are marked for depths of 6, 8, 10, 11.5, 13 and 16mm, and are equipped with a podium that allows the connection of MIS drill stoppers. All MIS drills have a 120°C cutting degree. The sharpness

and high quality of the drills allow for up to 30 uses. Careful use of sharp drills will ensure atraumatic drilling procedures, and minimal heat generation.

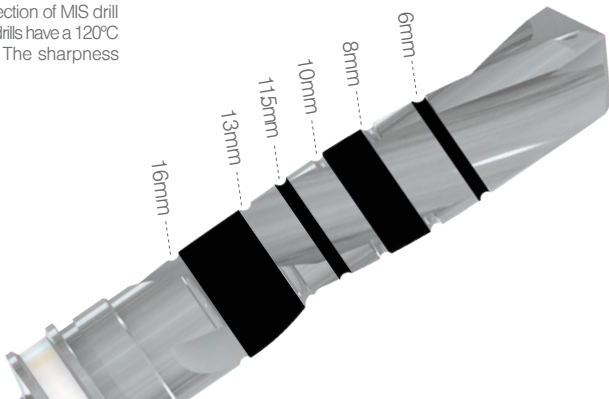

Drill Stopper

MIS offers drill stoppers to enable simple and accurate depth control.

The SEVEN drill stopper kits (MK-SDS06, MK-SDS08, MK-SDS10, MK-SDS11, MK-SDS13) are a series of kits, each used for one specific implant length: 6, 8, 10, 11.5 or 13mm.






For most commonly used implant lengths 3.75 or 4.2, MIS offers a single assorted kit - the SEVEN drill stoppers kit Standard platform (MK- BS001), which includes all stoppers required for safe placement of Standard platform implants.

SEVEN Drill Stoppers Kit:
(MK-SDS06, MK-SDS08, MK-SDS10, MK-SDS11, MK-SDS13)



SEVEN Drill Stoppers Kit Standard Platform:
(MK-BS001)



	Diameter	Length
	Ø2.80mm	37.5mm
	Ø3.20mm	37.5mm
	Ø4mm	38.2mm
	Ø4.50mm	38.2mm
	Ø5mm	38.2mm

Drills
Color Code



Color-coding is used for easy identification of drills or implants, diameters as follows:

Yellow

Implant Ø3.30 | Drill Ø2.40

Red

Implant Ø3.75 | Drill Ø2.80

Blue

Implant Ø4.20 | Drill Ø3.20

Green

Implant Ø5 | Drill Ø4

White

Implant Ø6 | Drill Ø4.50/5Ø


Drills

Drill Indications

Important!


Please note that the apical tip of all MIS twist drills is up to 0.5mm longer than the depth of the corresponding implant.

This should be taken into account during the planning phase.

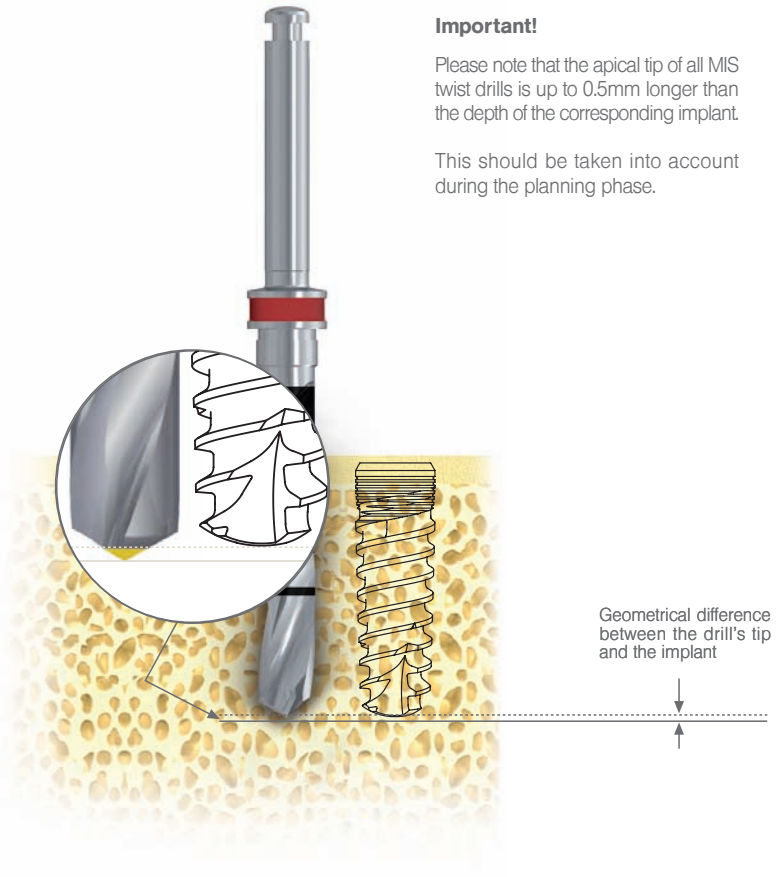


Depth Verification

Depth verification can be done by the use of body try-in tools (MT-BTTxx). The laser markings correspond to those on the drills and allow a safe, easy way to ensure the required depth is achieved.

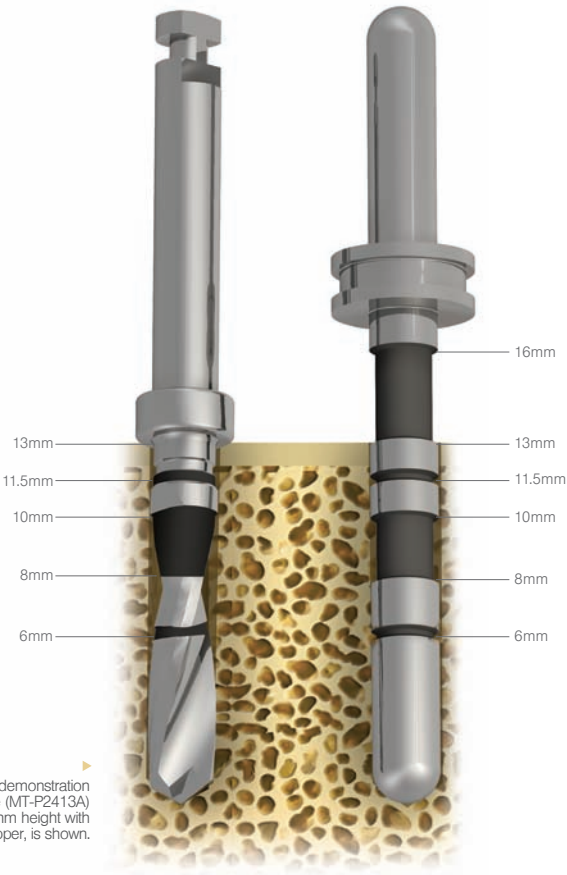

Drills
Drill Overview

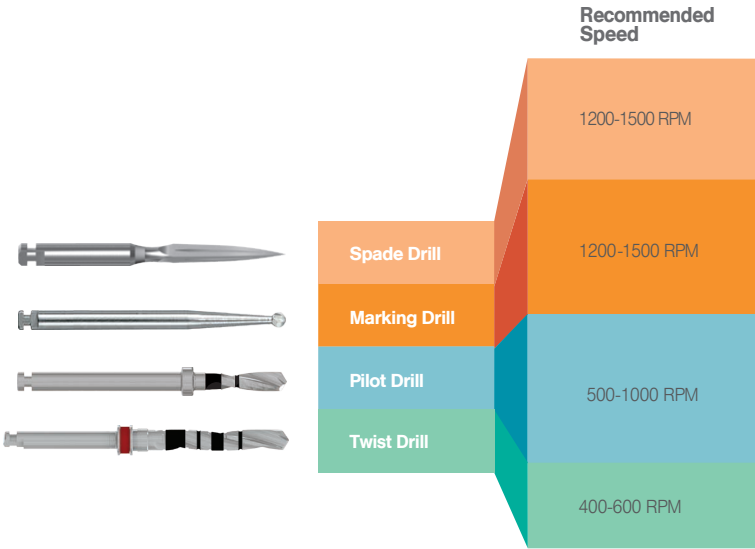

Length & Diameter

The spade drill has a diameter of Ø1.9mm and a sharp tip. The spade drill is 27.5mm in length and made of stainless steel.

The marking drill supplied is 34mm in length and 1.90mm in diameter.

SEVEN pilot drills come in six different lengths: 6, 8, 10, 11.5, 13 and 16mm and are equipped with a stopper to simplify the drilling procedure.

Twist drills come in a variety of diameters and lengths.

Aim of Use

The spade drill is used to mark a reference point for further drills. It is especially useful in immediate placement procedures.

The marking drill is used for creating a reference point in the center of the ridge, and to mark the drilling location for further drilling.

Pilot drills are the first invasive drills used for the preparation of a fixture site. The Pilot drills are length specific to ensure precise drilling depth.

Twist drills are used to widen the osteotomy. They are NOT length specific, and have laser markings for 6, 8, 10, 11.5, 13 and 16 mm implants. The use of stoppers is highly recommended when using twist drills.

SEVEN Final Drill

Final Drill for implant diameters


Ø3.30

Ø3.75

Ø4.20

Ø5


Ø6

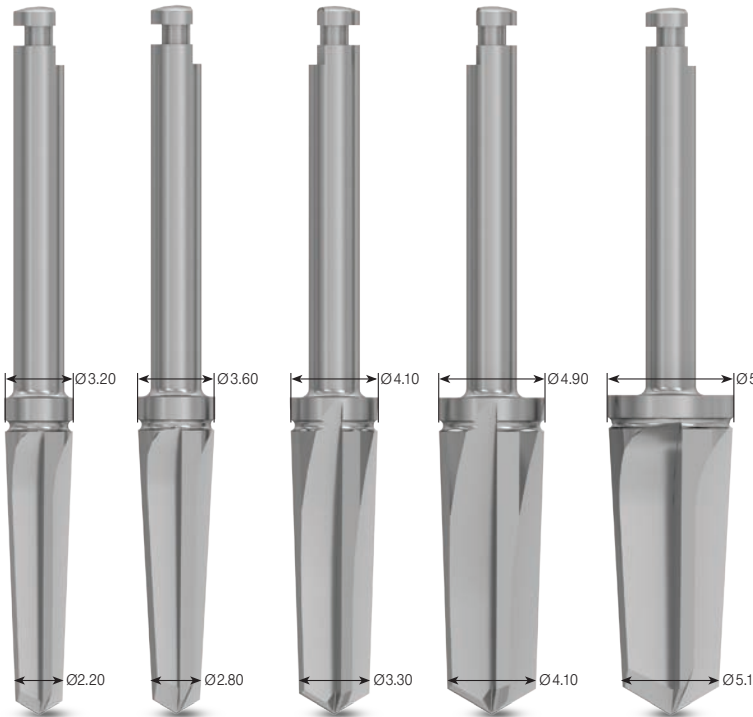

SEVEN

Special Final Drill

The specially designed single-use final drill is recommended for use in bone types 1 and 2 for 6, 8, 10, 11.50, 13 and 16mm SEVEN implants in order to prevent pressure on the implant neck. The special final drill is supplied with every implant, allowing for a shorter, safer drilling procedure. Recommended drilling speed is 200-400 Rpm.

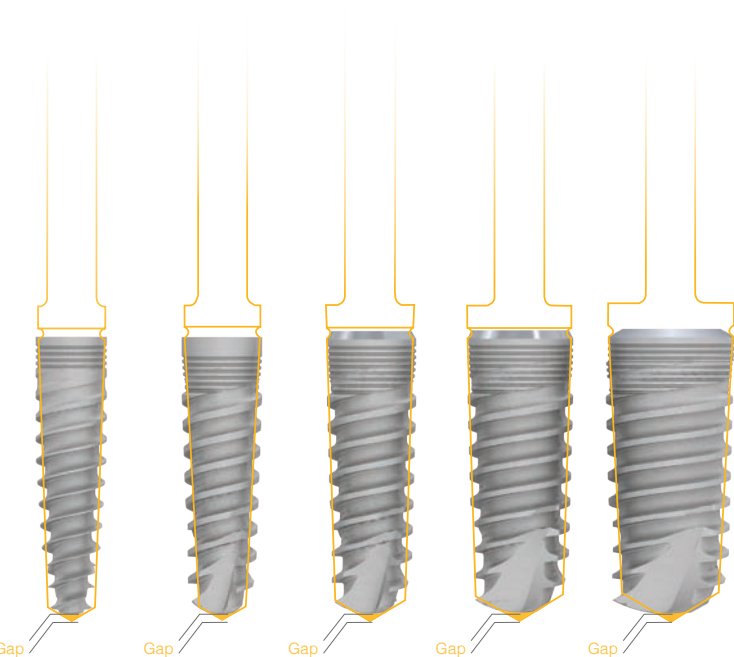


Drills

Countersink Drills

Countersink (MT-GDN33, MT-GDN50)

A Countersink drill is used to widen the entrance area of the osteotomy, to prevent extensive pressure on the implant neck. Depth marks of 3.75 and 4.20mm appear on the Standard platform countersink drill (MT-GDN33), and 5 and 6mm marks appear on the Wide platform countersink drill (MT-GDN50). Recommended drilling speed is 200-500 RPM.

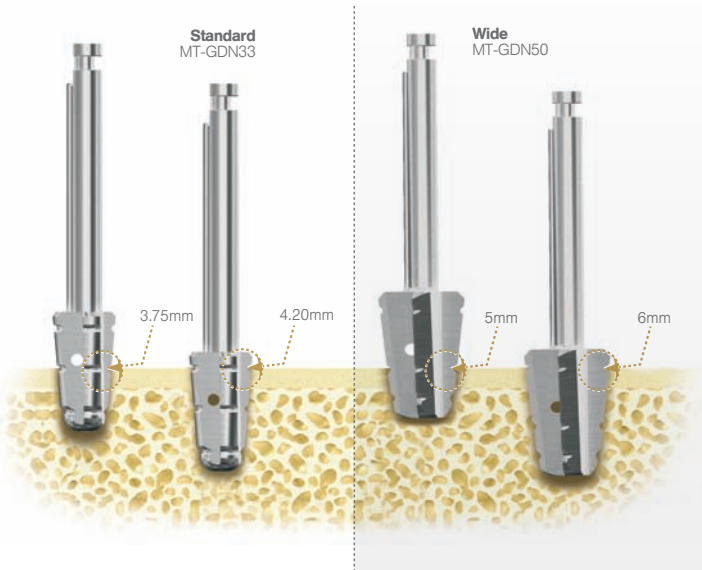

Drills

Ceramic Drills

Ceramic drills feature reduced vibration, smooth operation and continuous substance removal.

MIS ceramic drills are made of a high performance mixture of zirconium dioxide (zirconia) and aluminum oxide (alumina) ceramics. The mixture of these two materials provides MIS ceramic drills with an above-average bending strength of 2,000 MPa. In comparison, the bending strength of zirconium oxide ceramic, used in the manufacturing of root posts is 1,200 Mpa.

Advantages: Metal-free, biocompatible, corrosion-free



MT-CRD21
Marking Drill

Dimensions: Ø2.10mm
Length 28.5mm

Material: Zirconia-
alumina ceramic



MT-CRD20
Pilot Drill

Dimensions: Ø2mm
Length 33.5mm

Material: Zirconia-
alumina ceramic



MT-CRD28
Twist Drill

Dimensions: Ø2.80mm
Length 35mm

Material: Zirconia-
alumina ceramic

Drills Drills Maintenance

Correct and careful maintenance of MIS drills is extremely important. Damage to drill tips can cause significant impairment of drill function. The following are detailed instructions for proper maintenance.



Instructions for Maintenance of Drills Prior to First Use

Stage 1: Cleaning and Rinsing - Drills should be dipped in appropriate detergent, rinsed, and dried. The use of an ultrasonic bath is highly recommended.

Stage 2: Sterilization - Drills should be sterilized in an autoclave at 134°C (273°F), at a pressure of ≈315 Kpa for 6 minutes or in a pre-vacuum autoclave at 132°C (270°F) for 4 minutes. Do not exceed 134°C.

Stage 3: During Use - Drills should be soaked in a sterile saline solution until the cleaning stage.



Instructions for Cleaning and Storage of Drills After Use

Stage 1: Cleaning - Drills should be brushed with detergent to remove any remaining blood or tissue.

Stage 2: Ultrasonic cleaning - Drills should be cleaned in an ultrasonic bath with appropriate detergent. Note: during ultrasonic cleaning, contact between drills should be avoided.

Stage 3: Rinsing - Drills should be rinsed under running water and dried.

Stage 4: Sterilization - Drills should be sterilized in an autoclave at 134°C (273°F), at a pressure of ≈315 Kpa for 6 minutes or in a pre-vacuum autoclave at 132°C (270°F) for 4 minutes. Do not exceed 134°C.


Stage 5: Storage/Use - Store kits in a cool and controlled environment. Please note that sterilization may expire after a certain time. If kits have been stored for a prolonged period resterilize them to use.

Drills **Drills** **Maintenance**



Recommendations

- Cutting tools should be used for a maximum of 30 uses.
- Distilled water should be used in order to avoid surface stains.
- 132°C (270°F) for 4 minutes: pre-vacuum autoclave for Instruments / drills / kits.
- 134°C (273°F) for 6 minutes: Autoclave for Instruments / drills

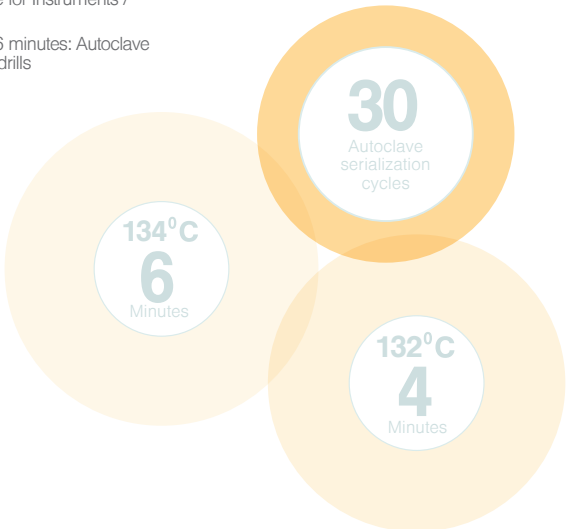




Surgical & Prosthetic Tools.

- 66. Mono-Block Ratchet Wrench
- 68. Implant Site Depth Probe
- 69. Implant Direction Indicator
- 70. Implant Extraction Keys
- 72. Specialized Surgical Tools
- 74. Friction Fit
- 76. SOS Broken Screw Kit
- 78. Screw Tests
- 79. Maintenance

Ratchet **Mono-Block Ratchet Wrench**

The new ratchet is a mono-block instrument with a unique mechanism that simplifies use and cleaning. To prevent damage to the mechanism, it is critical that the ratchet is used only with keys and adapters that are specifically designed for it. The ratchet wrench can be used for implant placement and tightening or loosening screws.

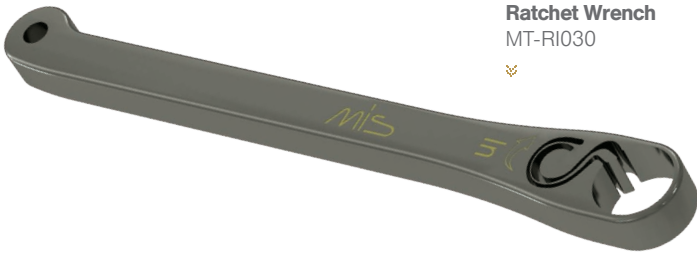

Ratchet Wrench
MT-RI030



Warnings

It should be emphasised that MIS recommends the use of a torque controlled driver whenever possible.

The ratchet wrench MT-RI030 may transfer torque levels that do not correlate to the recommendations specified for implant placement or screw fastening.

Excess loads may result in damage to

implants, components, screws, the wrench itself and even to the bone-to-implant interface.

Instrument Maintenance

- The device is not sterile.
- Cleaning and sterilization are required prior to first use.
- Clean instrument with running water to remove any blood or tissue immediately after use.


Cleaning and Disinfection:

- Immerse instrument in an approved cleaning/disinfecting solution.
- Use of an ultrasonic cleaner is highly recommended.
- DO NOT USE agents containing high concentration of chlorine or agents containing oxalic acid.
- Use distilled water to prevent water stains.


Sterilization

- All dental instruments must be sterilized prior to each use.
- The device is delivered non-sterile.
- Before use, the device must be sterilized by autoclave, at 134°C (273°F), at a pressure of ≈ 315 Kpa for 6 minutes or by pre-vacuum autoclave at 132°C (270°F) for 4 minutes. Do not exceed 134°C.

User Instructions

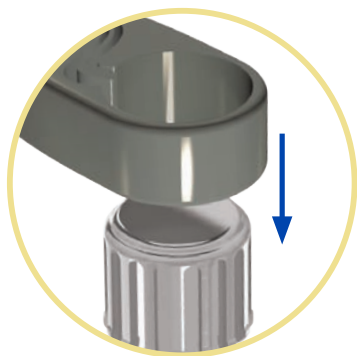

Store the ratchet on its own, not attached to any tools.

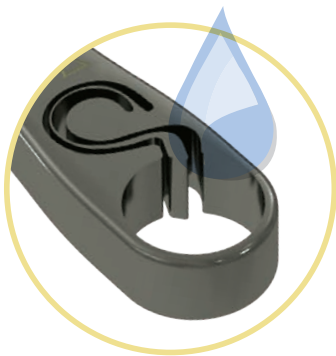


Clean thoroughly immediately after use.

Surgical Tools

Implant Site Depth Probe

Implant Site Depth Probe MT-BTI10

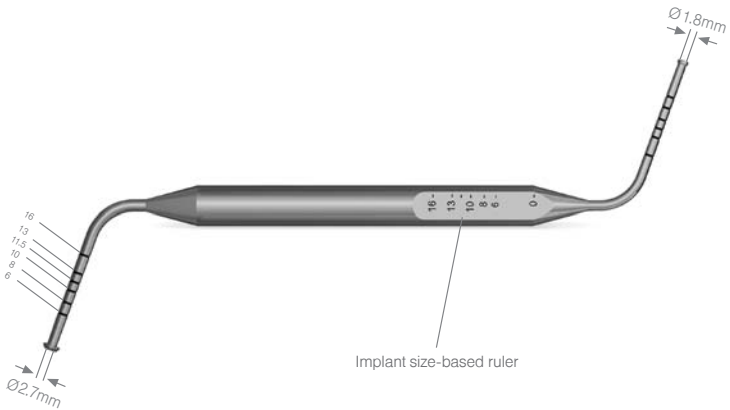

Features

The probe enables quick and easy measurements and examination of a prepared implant site, for each step of the procedure.

Marked depths: 6, 8, 10, 11.5, 13 and 16mm.
The depth probe includes an apical flat section

to ensure accurate placement within the osseotomy.


Dimensions: Ø1.80 / Ø2.70mm. Total length: 100mm.

Surgical Tools

Implant Direction Indicator

Implant Direction Indicator MD-PF375/ MN-PF330


The Direction Indicator is placed in the osteotomy to check direction and depth of the implant bed. When more than one implant is placed, the Direction Indicator is used to verify parallelism of the other implants.

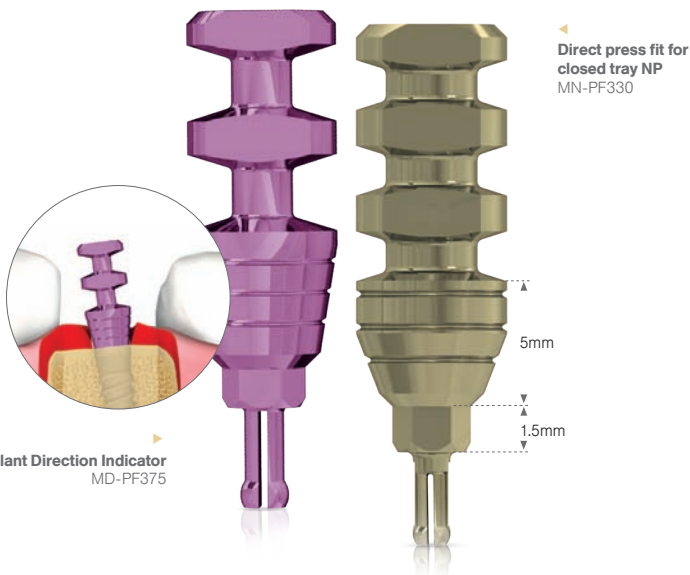

Surgical Tools

Implant Extraction Keys

The Implant Extraction Keys are designed for the extraction of mountless Standard or Wide platform implants, and can be used manually or with a ratchet. Each key consists of two components: the body, which includes a standard hex. and a key screw, that passes through the body to allow a firm connection between implant and key; for a safe and simple implant extraction. It is recommended to dismantle both components (key body and screw), prior to cleaning and sterilization.

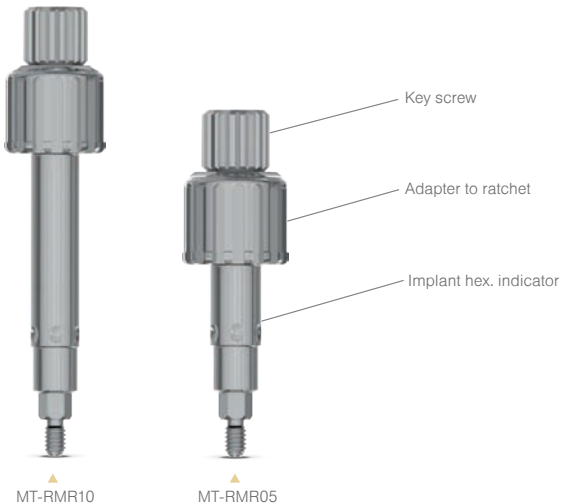


Direct Hand and Ratchet Hex. Key

MT-RMR05 / MT-RMR10

Step

1.

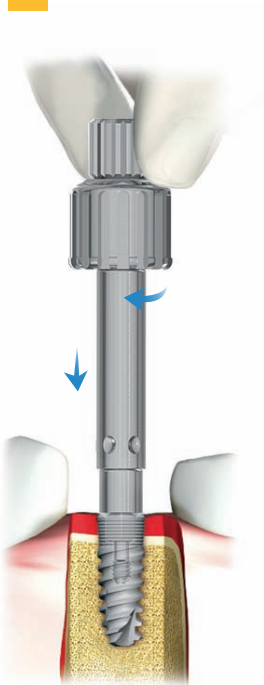


By Hand

Tightening the screw to the implant

Step

2.

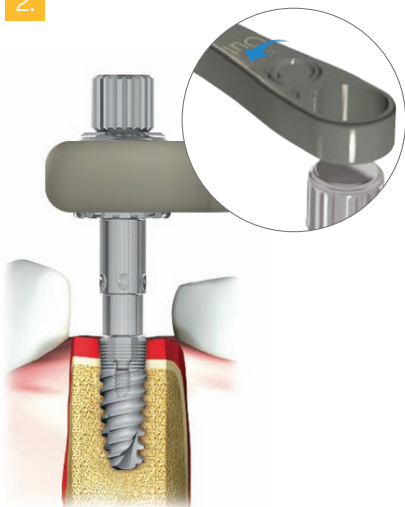


By Ratchet

Ratchet is connected to top of the key in order to pull the implant out


Surgical Tools
**Specialized
Surgical Tools**

SEVEN Insertion Tools

Insertion tools are available in short and long versions, for manual, ratchet or motor options.

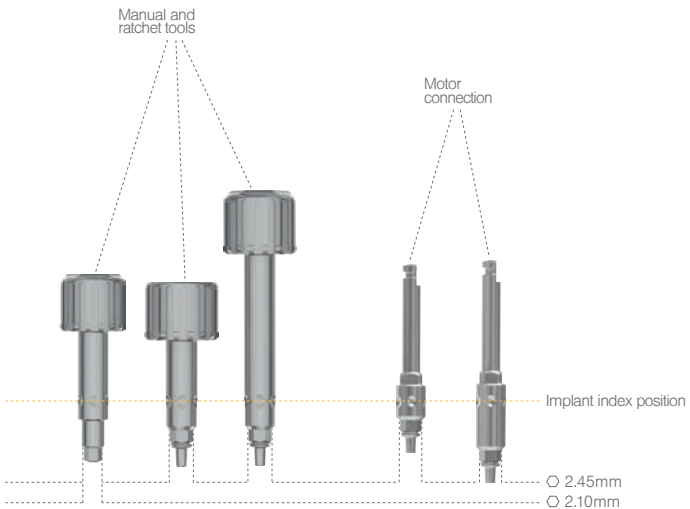

Insertion Options

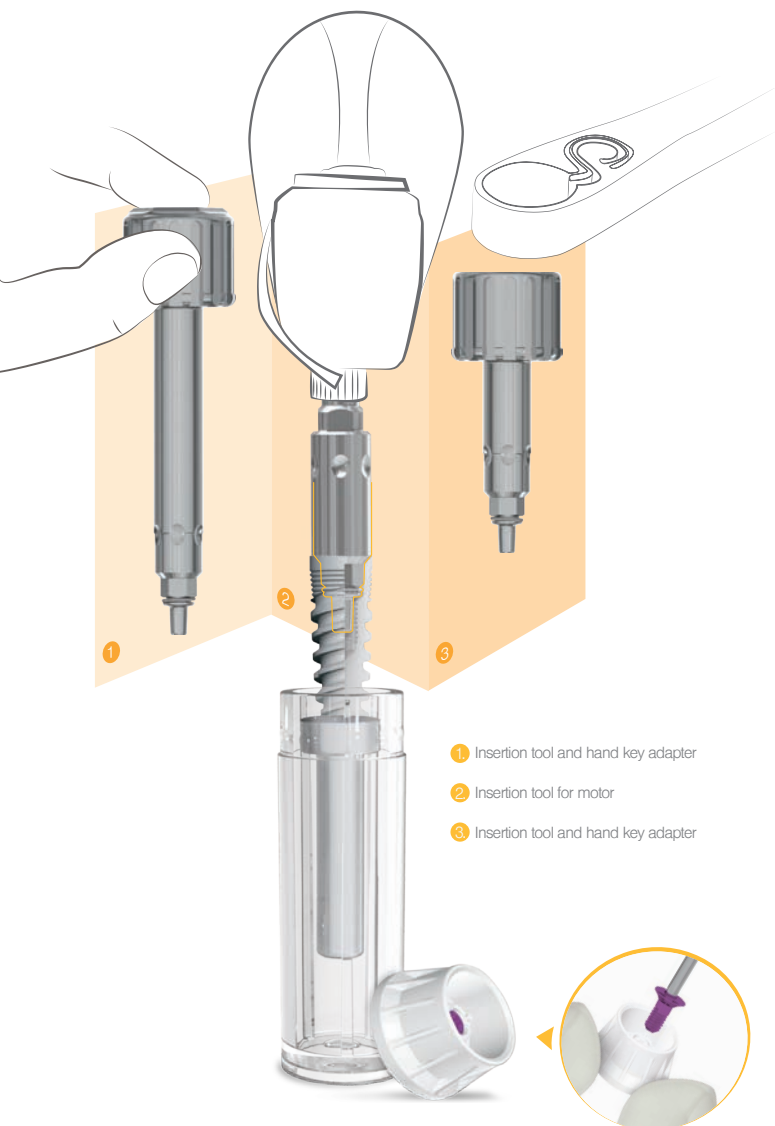


The same concept is applicable for Wide platform tools.

Prosthetic Tools
**Friction Fit
extractor**


Friction Fit

MT-RE172/ MT-RE160

The friction fit extractors are designed to separate the friction fit abutments from the implant. The extractors are color-coded, Blue for Standard/Wide abutments and Yellow for Narrow abutments.

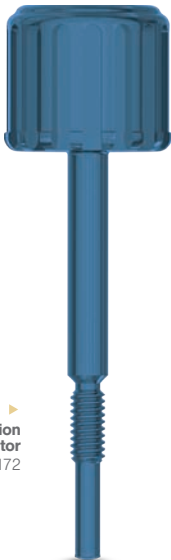

▶
Int. connection
abutment extractor
MT-RE172


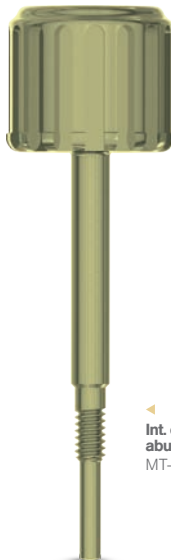


◀
Int. connection
abutment extractor, NP
MT-RE160



Mode of action

The extractor key applies vertical load parallel to the long axis of the implant. Thus it can release a "locked" abutment from an implant.

For Standard / Wide Implants

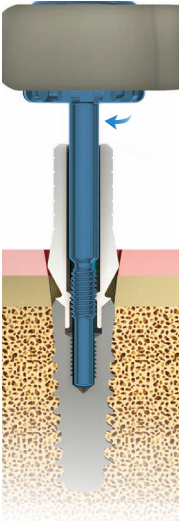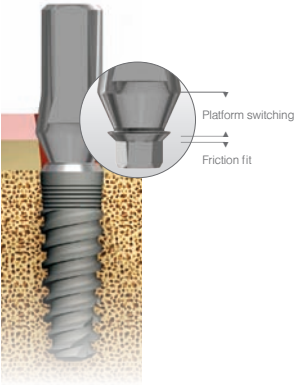

For Narrow Implants

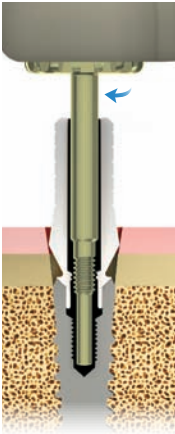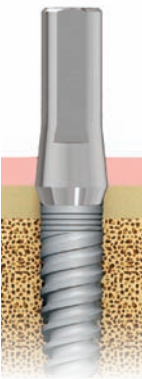

Prosthetic Tools
**SOS Broken
Screw Kit**

SOS Broken Screw Kit

MT-TF172 / MT-RT001/ MT-HW001

The SOS Broken Screw Kit was designed to facilitate the removal of a broken screw from within an implant.



▶ **SOS Broken Screw Kit**
MK-0041

SOS Tools



Thread Former
MT-TF172



Retriever
MT-RT001




Hand Wrench
MT-HW001

Instructions for use:



1.

- A. Connect the retriever to a micromotor.
- B. Adjust the micromotor to low speed (15-25 RPM), max. torque and in reverse mode.

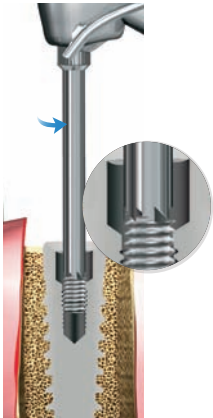

2.

- A. Apply mild pressure with the retriever on the top of the broken screw.
- B. While maintaining pressure, activate the motor. This action should release the screw. If the screw is still not released, apply intermittent pressure on the screw.




3.


- If internal threads are damaged:
- A. Use the thread former with care.
- B. Be sure to align the thread former parallel to the long axis of the implant.
- C. Always start by using a hand wrench. Apply gentle but firm force while turning the thread former parallel to the long axis of the implant in a clockwise direction. Release the pressure at the end of each complete turn by turning it 30° in a reverse direction, and repeat the action as needed.
- D. In instances where greater torque is needed, a ratchet may be used.

Surgical Tools
Screw Tests

Tensile Test of Dental Screws

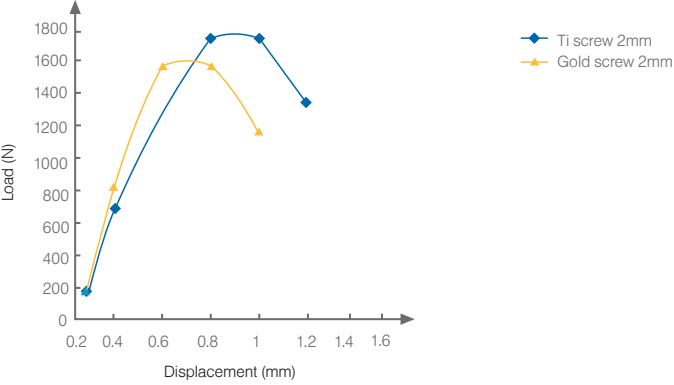

Fatigue Test of Dental Screw

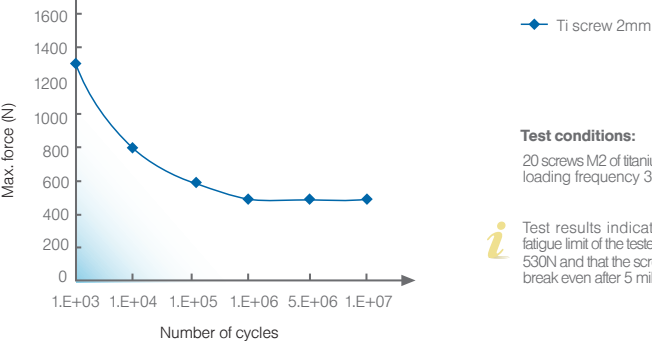

Test conditions:
20 screws M2 of titanium grade 5
loading frequency 30Hz.

i Test results indicate that the fatigue limit of the tested screws is 530N and that the screws will not break even after 5 million cycles.

Maintenance

The wide variety of MIS surgical tools require careful maintenance:



Instrument maintenance:

MIS surgical instruments are delivered non-sterile, unless indicated otherwise.

Disinfection

- Immerse instruments immediately after use.
- Use approved agents only.
- Observe manufacturer's recommendations regarding concentration/time/material compatibility.
- Verify that detergents and cleaning agents don't contain oxalic acid and high rates of chlorine.
- Avoid extremely high temperature during cleaning and sterilization of the product.

Cleaning

- Remove all residues.
- Use an ultrasonic bath.
- Use anticorrosive cleaning agent.
- Thoroughly rinse away cleaning and disinfecting agents with running water.
- Use distilled water to prevent water spots.

Drying

Allow instruments to dry prior to sterilization.

Examination

- Perform a visual inspection.
- Dispose of damaged instruments.

Check for:

Broken or dull drill blades
Bent instruments
Corrosion

Sterilization

Surgical instruments must be sterilized before use by autoclave, at 134°C (273°F), a pressure of ≈315 Kpa for 6 minutes or by pre-vacuum autoclave at 132°C (270°F) for 4 minutes. Do not exceed 134°C. Kit has to be sterilized by pre-vacuum autoclave at 132°C for 4 minutes.

Storage

Store in a dry, dust-proof area. Keep instruments separated from chemicals. Resterilize prior to use, if instruments have been stored for a prolonged period of time.





Packaging.

- 82. Implant Packaging
- 84. Implant Identification Codes
- 85. Implant Data Label
- 86. Implant Package Handling
- 92. Planning Transparency
- 93. Symbols

Packaging **Implant Packaging**

The MIS packaging system is designed for simple and easy use. All implant boxes feature distinctive colors, large typeface, clear data labels and a pull tab for quick opening. Box dimensions are designed for compact, space-saving storage.

Individual Implant Package

Following the "Make It Simple" philosophy, MIS is proud to be the first to include a sterile single-use final drill with every SEVEN implant, to ensure a safe and precise surgical procedure.



Implant package



▲ 10 Implant Package

A convenient 10 implant package is available. The box is ideal for storage in drawers or cabinets for easy identification of implant type, diameter and length.



▲ Implants are packed without a mount, for ease of use and a faster placement procedure.

Double Container Sealing System

To ensure that implants are sterile, and to prevent surface contamination, each implant is stored in a titanium sleeve within an internal plastic tube. This tube is held in a larger sealed outer tube, marked with all relevant information. The inner tube is therefore sterile, and can be brought into the sterile surgical field whenever needed.



Cover screw




▲ Implant




Packaging Implant Identification Codes

For easy identification of implant diameter, length and platform, the package and cap of each outer tube is coded as follows:

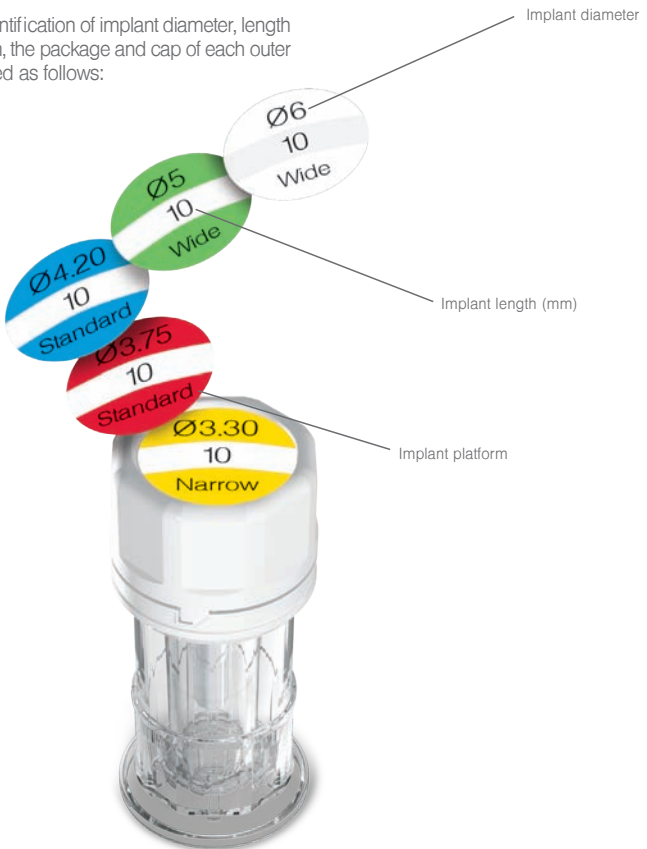

Packaging Implant Data Label

Each package contains three data labels, which include all required information relevant to the implant. The following image illustrates the label and its contents:

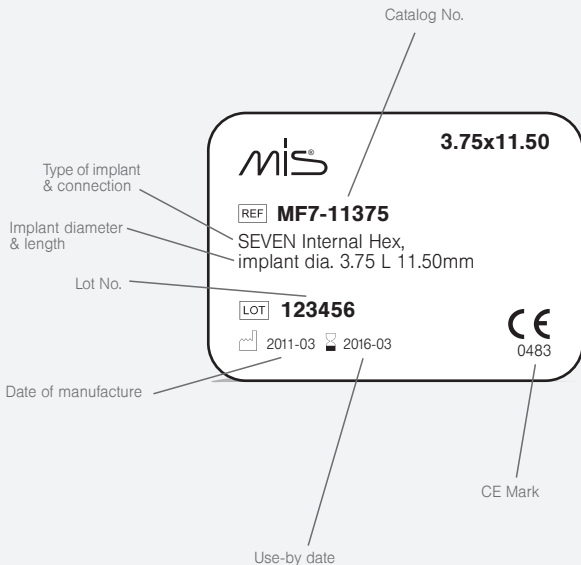

Packaging **Implant Package Handling**

Both physical and visual inspection of the implant package is required prior to use. This ensures that the correct implant model and dimensions are being used for the selected site.



Fig. 1

Open the box by pressing on the marked dotted line, and remove the outer tube from the box.



Fig. 2

Open the outer tube by turning the cap counter-clockwise. Drop the sterile inner tube into the sterile field.



Fig. 3

The implant is held by the titanium sleeve. To expose the implant - hold the tube with the titanium sleeve facing up. Rotate and pull to open the upper cap.



Use one of the following three options to remove the implant from the inner tube:

Fig. 4

Contra-angle hand piece

Packaging
**Implant
Package
Handling**

OPTION 2



Fig. 5
Ratchet

OPTION 3



Fig. 6
Implant extraction



Fig. 7

Remove the cover screw from the inner tube cap using the key.

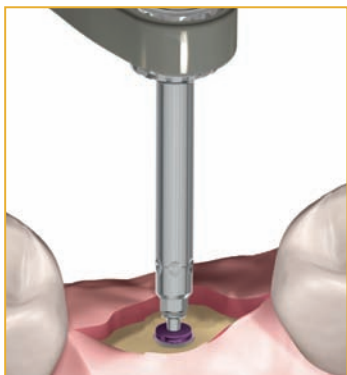


Fig. 8


Begin tightening the screw.



Fig. 9

The data labels should be used within the medical chart.

Packaging
**Implant
Package
Handling**



Inner Tube



Outer Tube




Planning Transparency

MIS offers a planning transparency, illustrating the full SEVEN implant range. It includes two sets of images: one actual size 1:1, and the other at a magnification of 125%; for use with panoramic radiographs that include a similar inherent magnification. In addition, the transparency includes a 1:1 ruler.

By aligning the appropriate section of the transparency on a radiograph, the clinician can choose the optimum implant diameter and length, as part of the planning process.

Cat No. **MC-SEVIN**

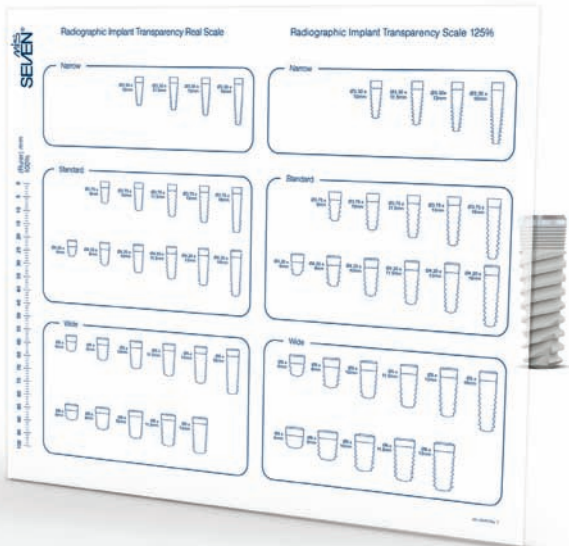



Symbols

Key to symbols that appear on labels and instruction leaflets:

	Batch code		Manufacturer
	Catalog number		Do not resterilize
	For single use only		Do not use if package is damaged
	Attention, see instructions for use		Authorised representative in the European community
	Date of manufacture		Use-by date
	Sterilized using gamma irradiation		



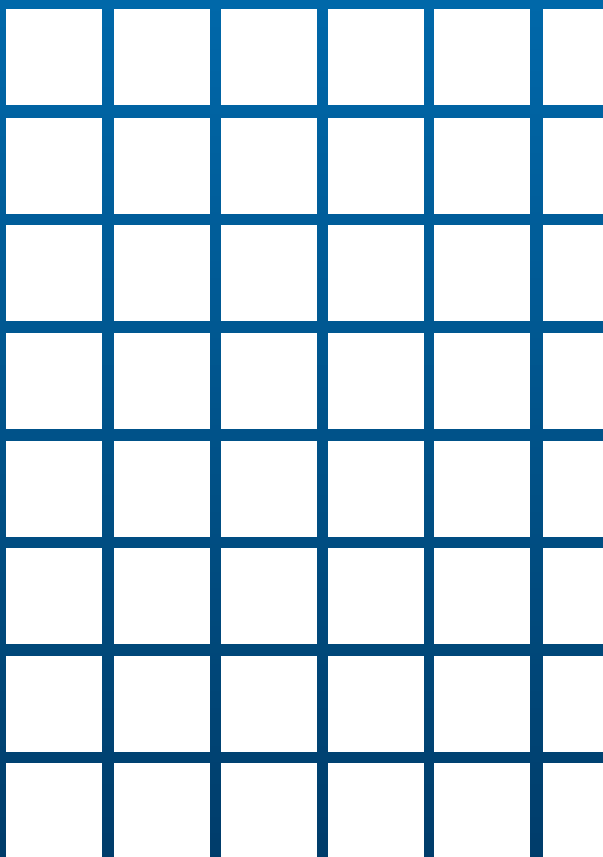

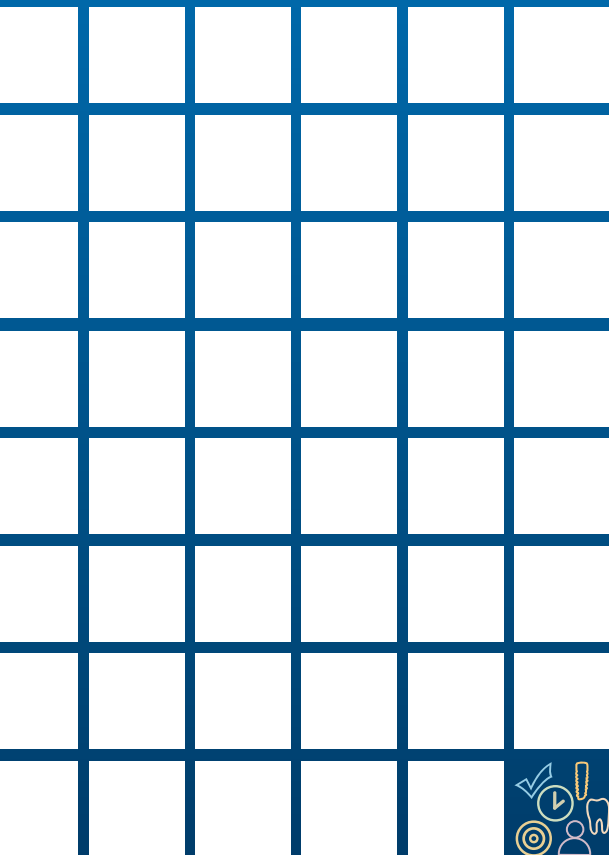

All rights reserved. No part of this publication may be reproduced, transcribed, stored in an electronic retrieval system, translated into any language or computer language, or be transmitted in any form whatsoever, without the prior written consent of the publisher. Warning: Only a licensed dentist should use these products.



MIS Implants Technologies Ltd.
www.mis-implants.com

The MIS Quality System complies with International Quality Standards: ISO 13485:2003 - Quality Management System for Medical Devices, ISO 9001:2008 - Quality Management System and CE Directive for Medical Devices 93/42/EEC. MIS products are cleared for marketing in the USA and CE approved.